



CERTIFICATE OF ACCREDITATION

The ANSI National Accreditation Board

Hereby attests that

Cal-Chek Canada, Inc.
250 Governor's Road
Dundas, ON L9H 3K3
Canada

Fulfills the requirements of

ISO/IEC 17025:2017

In the field of

CALIBRATION

This certificate is valid only when accompanied by a current scope of accreditation document.
The current scope of accreditation can be verified at www.anab.org.

A handwritten signature in black ink, appearing to be 'J. Stine', is positioned above a horizontal line.

Jason Stine, Vice President

Expiry Date: 11 August 2028
Certificate Number: L1001-1



This laboratory is accredited in accordance with the recognized International Standard ISO/IEC 17025:2017.
This accreditation demonstrates technical competence for a defined scope and the operation of a laboratory
quality management system (refer to joint ISO-ILAC-IAF Communiqué dated April 2017).

SCOPE OF ACCREDITATION TO ISO/IEC 17025:2017

Cal-Chek Canada, Inc.
250 Governor's Road
Dundas, ON L9H 3K3
Kevin Newitt 905-628-4636

CALIBRATION

ISO/IEC 17025 Accreditation Granted: **31 July 2026**

Certificate Number: **L1001-1**

Certificate Expiry Date: **11 August 2028**

Length – Dimensional Metrology

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Extrusion Plastometers ¹ (Melt Indexers, Melt Flow Indexers)			
Piston Foot Length	(0.2 to 0.3) in	1 500 µin	Per ASTM D1238 using Caliper
Piston Foot Diameter	(0.3 to 0.4) in	120 µin	Micrometer
Automatic Timing Switch Travel	(0.2 to 1.2) in	1 200 µin	Micrometer Head
Go/No-Go Gauge	(0.082 to 0.083) in	110 µin	Micrometer
Cylinder Bore Diameter	(0.3 to 0.4) in	180 µin	Bore Gauge, Ring Gauge
Die/Orifice Length	(0.3 to 0.4) in	120 µin	Micrometer
Die/Orifice Bore Diameter	(0.082 to 0.083) in	120 µin	Go/No-Go Gauge
Extensometer Systems ^{1,2} (Strain Instruments, Extensometers, Deflectometers)	(0.000 1 to 1) in	(94 + 27L) µin	Per ASTM E83 using Cal-60 Calibrator
	(0.005 to 17) in	(18 + 59L) µin	Gauge Blocks

Length – Dimensional Metrology

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Displacement Measuring Systems and Devices ^{1,2}	(0.0001 to 1) in	(150 + 540L) μ in	Per ASTM E2309/E2309M using LVDT Calibrator
	(0.005 to 3) in	(1 100 + 180L) μ in	Dial Gauge
	(0.005 to 17) in	(18 + 59L) μ in	Gauge Blocks

Mass and Mass Related

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Force Testing Machines ^{1,2} Compression	(0.1 to 61) lbf (61 to 600 000) lbf	(0.001 1 + 0.000 3M) lbf 0.11 % of Applied Load	Per ASTM E4, ASTM C39, CSA A23.2-9C using Dead Weights Load Cells and Display
Force Testing Machines ^{1,2} Tension	(0.1 to 61) lbf (61 to 300 000) lbf	(0.001 1 + 0.000 3M) lbf 0.11 % of Applied Load	Per ASTM E4 and CSA A23.2-9C using Dead Weights Load Cells and Display
Brinell Hardness Tester ¹ Force	(500 to 3 000) kgf	3.9 kgf	Direct Verification using Brinell Proving Ring per ASTM E10.
Brinell Hardness Testers ¹	Low Medium High	0.9 HBW 5.2 HBW 7.8 HBW	Indirect Verification using Standardized Test Blocks per ASTM E10.
Rockwell Hardness Testers ¹	HRA Low Medium High HRBW Low Medium High	0.31 HRA 0.2 HRA 0.18 HRA 0.33 HRBW 0.28 HRBW 0.4 HRBW	Indirect Verification using Standardized Test Blocks per ASTM E18.

Mass and Mass Related

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Rockwell Hardness Testers ¹	HRC		Indirect Verification using Standardized Test Blocks per ASTM E18.
	Low	0.38 HRC	
	Medium	0.33 HRC	
	High	0.32 HRC	
	HREW		
	Low	0.57 HREW	
	Medium	0.56 HREW	
	High	0.56 HREW	
	HRFW		
	Low	0.54 HRFW	
Rockwell Superficial Hardness Testers ¹	Medium	0.46 HRFW	Indirect Verification using Standardized Test Blocks per ASTM E18.
	High	0.47 HRFW	
	HRRW		
	118 HRRW	0.32 HRRW	
	HRLW		
	105 HRLW	0.37 HRLW	
	HR15N		
	Low	0.44 HR15N	
	Medium	0.24 HR15N	
	High	0.22 HR15N	
Rockwell Superficial Hardness Testers ¹	HR15TW		Indirect Verification using Standardized Test Blocks per ASTM E18.
	Low	0.36 HR15TW	
	Medium	0.37 HR15TW	
	High	0.32 HR15TW	
	HR30N		
	Low	0.41 HR30N	
	Medium	0.19 HR30N	
	High	0.30 HR30N	
	HR30TW		
	Low	0.52 HR30TW	
Rockwell Superficial Hardness Testers ¹	Medium	0.31 HR30TW	Indirect Verification using Standardized Test Blocks per ASTM E18.
	High	0.33 HR30TW	
	HR45N		
	Low	0.54 HR45N	
	Medium	0.58 HR45N	
	High	0.29 HR45N	

Mass and Mass Related

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Rockwell Superficial Hardness Testers ¹	HR45TW Low Medium High HR15YW 90 HR15YW	0.70 HR45TW 0.61 HR45TW 0.46 HR45TW 0.98 HR15YW	Indirect Verification using Standardized Test Blocks per ASTM E18.
Leeb Hardness Testers ¹	(300 to 900) LD	9.4 LD	Indirect Verification using Standardized Test Blocks per ASTM A956.
Vickers Hardness Testers ¹	(100 to < 240) HV (240 to 600) HV > 600 HV	1.8 HV 5.2 HV 7.7 HV	Indirect Verification using Standardized Test Blocks per ASTM A92 and ASTM E384.
Knoop Hardness Testers ¹	(100 to < 250) HK (250 to 650) HK > 650 HK	1.9 HK 9.5 HK 14.4 HK	Indirect Verification using Standardized Test Blocks per ASTM A92 and ASTM E384.
Extrusion Plastometers ¹ Weights	(90 to 12 000) g	1.4 g	Bench Scales per ASTM D1238.

Thermodynamic

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Extrusion Plastometers ¹ Temperature Control Systems	(20 to 400) °C	0.08 °C	RTD Sensor and Display per ASTM D1238.


Time and Frequency

Parameter/Equipment	Range	Expanded Uncertainty of Measurement (+/-)	Reference Standard, Method, and/or Equipment
Extrusion Plastometers ¹ Time Devices/Timers	(10 to 600) s	1.3 s	Stopwatch per ASTM D1238.
Crosshead Speed ¹	(0.04 to 0.5) in/min	0.12 % of reading	Stopwatch and Displacement Measuring System per ASTM E2658.

Calibration and Measurement Capability (CMC) is expressed in terms of the measurement parameter, measurement range, expanded uncertainty of measurement and reference standard, method, and/or equipment. The expanded uncertainty of measurement is expressed as the standard uncertainty of the measurement multiplied by a coverage factor of 2 ($k=2$), corresponding to a confidence level of approximately 95%.

Notes:

1. On-site calibration service is available for this parameter, since on-site conditions are typically more variable than those in the laboratory, larger measurement uncertainties are expected on-site than what is reported on the accredited scope.
2. L = length in inches; M = force in lbf.

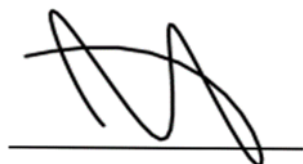

Jason Stine, Vice President

